

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

1102 3-1 700

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130180
Name	AW Anderson	ID#	2067
Agency	Seldovia PD	Date	7/9/11
Instrument Location	Seldovia PD	Phone #	234 7640
Alco S/N	X301530 BMB 8/11/11	Target Value	0.078
	X301530	High Pressure	500PSI
Alco Test Values	1st Alco 0.075	2nd Alco 0.075	
Signature	AW Anderson		

(OVER)

BMB 8/11/11

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 13 day of Aug, 2011


Nikki Roth
(Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

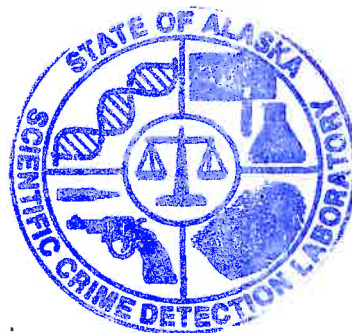

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130180 *BMB 7/12/11*

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

JULY 09, 2011

OPERATOR'S NAME:

BMB 8/1/11
ANDERSON, SM

OPERATOR'S NUMBER: 2467

SUBJECT'S LAST NAME:

SIXTY DAY VERIFICATION

SUBJECT'S FIRST NAME/MI:

N/A

D.L. #: 1234567890

DEPT/AGENCY: SOU1

CASE/REPORT: N/A

TEST TYPE: U

ALCO TARGET VALUE: .075

ALCO S/N: *X301520 BMB 8/1/11*

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 30.19 in

ALCO TARGET .075 20:07

BLANK TEST .000 20:08

INTERNAL STANDARD VERIFIED 20:08

ALCO TV 30.19 in .075 20:09

BLANK TEST .000 20:09

SUBJECT SAMPLE *BMB 8/1/11* .000 20:10

BLANK TEST .000 20:11

ALCO TV 30.19 in .075 20:11

BLANK TEST .000 20:12

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

JULY 09, 2011

TIME 20:04

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 30.19 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF8
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~
printtest()

